



Automated co-culture system for spatiotemporal analysis of cell-to-cell communication†

Cite this: DOI: 10.1039/c5lc00182j

Tino Frank and Savaş Tay

 Received 13th February 2015,
Accepted 7th April 2015

DOI: 10.1039/c5lc00182j

www.rsc.org/loc

We present a microfluidic co-culture system that generates localized and precisely formulated immune signals among a population of cells, enabling spatiotemporal analysis of paracrine signal transmission between different cell types. The automated system allows us to create temporally modulated chemical inputs that can be delivered to single signal-transmitting and receiving cells in a highly controlled way. Using this system we stimulated a single macrophage with brief pulses of bacterial LPS and observed the macrophage transmitted TNF signal propagating in a population of fibroblasts *via* NF- κ B activation. The signal receiving fibroblasts transformed the TNF signal into a spatiotemporally distributed NF- κ B output, recapitulating the initiation of immune response to bacterial infection.

Introduction

Global response to a local stimulus is ubiquitous in biological systems. A single cancer cell, for example, can kill an organism by forming a tumour,¹ localised enzyme production can create gradients of diffusive retinoic acid that patterns a growing organism,² the global heart pumping rate is controlled by a few local pacemaker cells,³ single bacteria can sense each other in close proximity and build a colony by quorum sensing⁴ and localized invading bacteria and viruses activate a global inflammatory response.⁵ Common to these examples is a spatially and temporally localized environmental input acting on a small group of cells, from where information spreads *via* cell–cell interactions to tissue by activating genetically encoded signalling pathways.

Many biological processes involve interactions between different cell types and subpopulations. A typical signalling scenario is presented in Fig. 1A. First, an immediate responder like a macrophage (cell type A) senses an environmental input like LPS from invading bacteria or an environmentally derived signalling molecule like TNF. This input is then processed using gene regulatory networks like NF- κ B (an important immune pathway⁶), and the appropriate response is computed by the first responder cell. In order to pass this information to neighbouring tissue cells, signalling mediators like inflammatory cytokines are secreted into the extracellular space. These cytokines are sensed by nearby responding cells, become processed and finally turned into a spatially distributed tissue level gene expression output

(Fig. 1A). Mediators can be transmitted *via* diffusion, gap-junctions or contact dependent signalling.⁷ The type, amplitude, duration and time course of the original signalling input determines the characteristics of cytokine secretion and cellular response. This information flow can lead to local reprogramming, differentiation, migration, apoptosis, proliferation of cells, or lead to further secretion of defined cytokines to elicit a global response. Importantly, these response characteristics may not only appear in a temporally modulated way,^{8,9} but they are also spatially organised. Spatial effects like tissue patterning or reorganisation are of immense importance in understanding biological phenomena like inflammation, and in modelling of signalling pathways.

Despite their importance, studies aimed at understanding the spatial aspects of cell signalling, especially with single-cell resolution, are few and far between. Traditionally used population assays are often obscured by “biological noise”, *i.e.* the naturally occurring cell-to-cell variability in isolated cell responses. Creating relevant signalling scenarios *in vitro* where single cells can be manipulated, tracked and quantitatively analysed is a technically challenging task.¹⁰ Many traditional methods are designed for population measurements in homogeneous (well-mixed) environments. For example, many insights into communication between pacemaker cells have been realised with an input delivered to the whole population.¹¹ The influence of positive feedback in yeast paracrine signalling was studied in a well-mixed environment,¹² thus ignoring the spatially inhomogeneous nature of signalling. To distinguish sender from receiver cells in bulk culture conditions, genetic modification had to be introduced, since defined spatial inputs have been lacking.¹³ There is consensus that heterogeneous cell environments like morphogen or cytokine gradients play major roles in developmental

Department of Biosystems Science and Engineering, ETH Zürich, Mattenstrasse 26, 4058 Basel, Switzerland. E-mail: savas.tay@bsse.ethz.ch

† Electronic supplementary information (ESI) available: 1 supplementary information document with 3 figures and 2 movies. See DOI: 10.1039/c5lc00182j

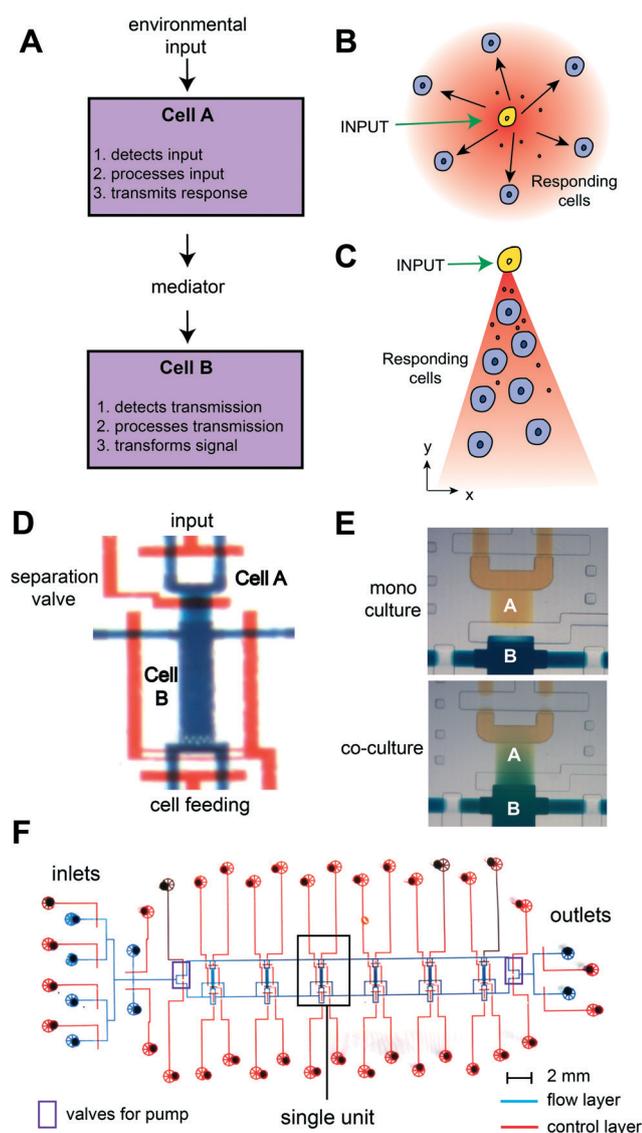


Fig. 1 (A) Typical one-way intercellular communication scenario, which we implemented *in vitro* in the current study. An environmental input like a pulse of pathogenic LPS is detected and processed by a first responder cell A (i.e. a macrophage), and the information is transmitted to resident tissue cells through secreted mediator molecules like cytokines. Cell B transforms this signal into a gene expression program. (B) First responder cells sense pathogen inputs locally, and transmit signals radially to a dense population of neighbouring cells *via* secreted molecules. (C) A one-dimensional geometry was used for technical implementation of one-way signal transmission on chip, which simplified cell manipulation and isolated signal delivery to first responder cells. A single macrophage is cultured in isolation, and responder cells are placed nearby in a linear arrangement. (D) Drawing of a single experimental unit that establishes the signalling arrangement described in C. First responder cell (cell A) is cultured in chamber A in isolation. Secondary responder cells (cell B) are cultured in an adjacent chamber separated by a membrane valve. Each chamber can be addressed independently using different fluid inlets, and cell-cell communication can be established by opening the separation valve. (E) Different culture modes on chip. In the monoculture the separation valve is closed. Co-culture mode allows cell-cell communication *via* secreted factors. (F) Up-scaled device with 6 independent experimental units. The violet boxes show the four valves for an on chip peristaltic pump (scale-bar = 2 mm).

biology¹⁴ and in inflammatory reaction to recruit more defender cells,¹⁵ or to conduct successful immune response.¹⁶ How signals evolve and propagate in such environments has not been studied in a spatiotemporally controlled manner. There is an immediate need for technical platforms that enable investigating spatiotemporal signal transduction to understand and model how signalling pathways control and process local information transfer, and how collective population behaviour emerges.¹⁷

Chemical stimulation of a single cell without stimulating the neighbouring cells is a necessary task when studying the common cell-to-cell communication scenario summarized in Fig. 1. To date, specific spatial stimulation was achieved by the use of optical or magnetic tweezers^{18,19} or photo-caged inducers,²⁰ which require advanced optical systems and their integration with standard cell culture experiments. Robotically controlled micropipettes can deliver local signals to cells, but it is difficult to prevent exposure to the neighbouring cells.²¹ Three-dimensional microfluidic systems can be used to bring localized signals to cells, but these systems require non-standard and complex fabrication methods.²² The complexity of the above-mentioned approaches may limit their application to high-throughput and controlled studies of cell-cell communication with single-cell resolution. Exclusive stimulation of single cells and subpopulations of cells using microfluidic parallel laminar flow has been previously shown.^{23,24} However, *in vivo* cell-cell communication is typically mediated by diffusion, and secreted signalling factors are quickly washed away when flow-based systems are used.

In this paper, we present an automated microfluidic co-culture device and integrated live-cell imaging system that can induce local signals on single cells and allow them to communicate with a second population of signal receiving cells in a precisely controlled way. Using a one-dimensional arrangement between different cell types, we were able to address a given cell type without affecting the others, and to study signal transduction between different populations (Fig. 1B and C). Using this system, we induced TNF secretion in a single macrophage by a temporally modulated local LPS input, and allowed this cell to communicate with a population of 3T3 fibroblasts, each expressing the fluorescent fusion protein p65/DsRed. These cells reacted by activating the canonical NF- κ B signalling pathway. The duration of the local LPS input pulse became converted into a spatial signalling range of NF- κ B activation among the 3T3 populations. We therefore showed how a single immune cell spatially controls a population of tissue cells through NF- κ B transcription factor oscillations in a highly realistic infection scenario established *in vitro*.

Materials and methods

Device design and fabrication

We designed, produced and implemented our device according to our standard protocol, which is reported elsewhere.²⁵ Briefly, we designed our two layer devices using AutoCAD

(Autodesk Inc., San Rafael, CA, USA). The designs were then printed on transparencies at 40 kdpi resolution (Fine Line Imaging, Minneapolis, USA). Moulds for PDMS casting were produced using standard soft-lithography. The channel network of control as well as the flow layer was produced with SU-8 3025 (Microchem, Westborough, MA, USA) on silicon wafers. For the flow layer we used AZ-50X (AZ Electronic Materials, Luxembourg) at valve positions. Both resists were spun to a height of 25 μm . For the flow layer, 72 g of PDMS (10:1; polymer:catalyst) was mixed, de-bubbled and poured over a TMCS treated silicon wafer. The PDMS was then cured for 60 min at 80 $^{\circ}\text{C}$. Inlet holes were then punched on the cured flow layer, which was then plasma treated and aligned to the flow layer that was spun at 2300 rpm with 5 g of PDMS (10:1). After a 2 h thermal bonding the holes for the control layer were punched and the chip was bonded to a PDMS coated coverslip and cured for 12 h at 80 $^{\circ}\text{C}$.

Chip control and operation

Our general purpose chip set-up and control apparatus is described in detail elsewhere.²⁵ In brief, our on-chip valves are controlled *via* external solenoid valves (Festo, Dietikon, Switzerland) that are managed through custom written LabVIEW software (National Instruments, Austin, USA). The software allows us to automate the experiments. To set up a chip, we first connect the PDMS chips to the solenoid valves *via* DI-water filled TYGON tubing (Milan, Satigny, Switzerland). The pressure is then slowly increased to 1.2 bar. Valve closing is checked visually. Afterwards, the flow layer is connected to waste and a container filled with PBS. Applying pressure (0.5 bar) to the PBS container but not the waste creates a pressure difference and therefore fluid flow. The flow layer gets then fully filled with PBS. In order to debubble the chip, outlet valves are first closed and air is fully pressed out through PDMS while PBS remains in the chip. The supply channels were then flushed with 10 mg mL⁻¹ pluronic acid (Millipore, Zug, Switzerland) for 3 min to prevent cell adhesion, followed by a 30 minute wash with PBS. Afterwards the cell culture areas are coated with fibronectin ($c = 50 \mu\text{g mL}^{-1}$, Millipore, Zug, Switzerland) for 60 min to ensure cell adhesion. PBS or medium then is flowed to replace the excess fluid in the cell culture chambers.

Cell culture and live-cell microscopy

We used NIH 3T3 p65^{-/-} cells with a p65-dsRed reporter gene as well as an H2B-GFP nuclear marker for tracking and analysis of NF- κ B nuclear localization. These cells are cultured in DMEM medium. To seed cells into the chip, cells are harvested at 80% confluence with trypsin from a dish. Half of the harvested cells are then resuspended in 1 mL of fresh DMEM and connected to the chip *via* pressurized vials. The seeding procedure is described in the Results and Discussion section (Fig. 2A). RAW 264.7 macrophages p65^{-/-} with a p65-GFP reporter gene as well as an H2B-dsRed nuclear marker are used as signal transmitting cells. These cells are

harvested at 75% confluence with Versene. The harvested cells were split, and resuspended (1:10) in fresh DMEM medium. 1 mL of the suspension was connected to the chip and seeded in the signal transmitter chamber.

To maintain long term culture on chip, a custom-made cell-culture and incubator system is used (Life Cell Imaging Service GmbH, Basel, Switzerland), consisting of a box surrounding the microscope where the temperature is kept constant at 37 $^{\circ}\text{C}$. To maintain 98% humidity and 5% CO₂ the PDMS chip is covered with a stage-top-incubator connected to a humidifier and a gas exchanger. For macrophage stimulation, we used ultrapure LPS (Invitrogen, San Diego, USA) at a concentration of 50 ng mL⁻¹ in cell culture medium. For blocking secreted TNF, we used anti-TNF antibody (Genwaybio, San Diego, USA) at a concentration of 100 $\mu\text{g mL}^{-1}$.

Image acquisition

For image acquisition a Nikon Ti-ECLIPSE microscope with an automated translation stage and a digital CMOS camera (ORCA-Flash 4.0, Hamamatsu, Japan) was used. The stage and image acquisition was controlled *via* the microscope's software (NIS Elements). A 4 \times objective (NA = 0.1, WD = 16500 μm) was used for setting up the chip, and image acquisition during experiments was realised by using a Nikon Plan Fluor 20 \times objective (NA = 0.5, WD = 82000 μm). The microscope's large image tool was used to stitch images. First a bright field image (it = 1 ms) is captured, and then the ds-Red channel is captured (it = 800 ms) followed by the GFP channel (it = 300 ms).

Data analysis

Images and data were analysed using MATLAB (Mathworks, Austin, USA). For tracking single cells, a custom written tracking algorithm was applied as described before.⁸ The algorithm extracts single traces of nuclear NF- κ B localization and reports cell positions as well. In brief, the nuclear area in each image is identified *via* the fluorescent nuclear marker GFP, and then the nuclear mean intensity of the p65-DsRed marker is measured, and plotted as a function of time.

Results and discussion

Device design for spatially localized stimulation of single cells and co-culture

We designed a microfluidic device that allows local stimulation of a single signal-transmitting cell independent of neighbouring cells, which also enables co-culture of the stimulated cell with other cell types. This ensures that each cell type is addressed independently, and signalling dynamics is not disturbed before exposure of cells to each other. In our device, cell-cell communication is mediated by diffusion of cell-secreted factors, and the position of signal sending and receiving cells is fixed by device geometry. If needed, the secreted factors can be flowed over the second population by the use of an on-chip peristaltic pump.

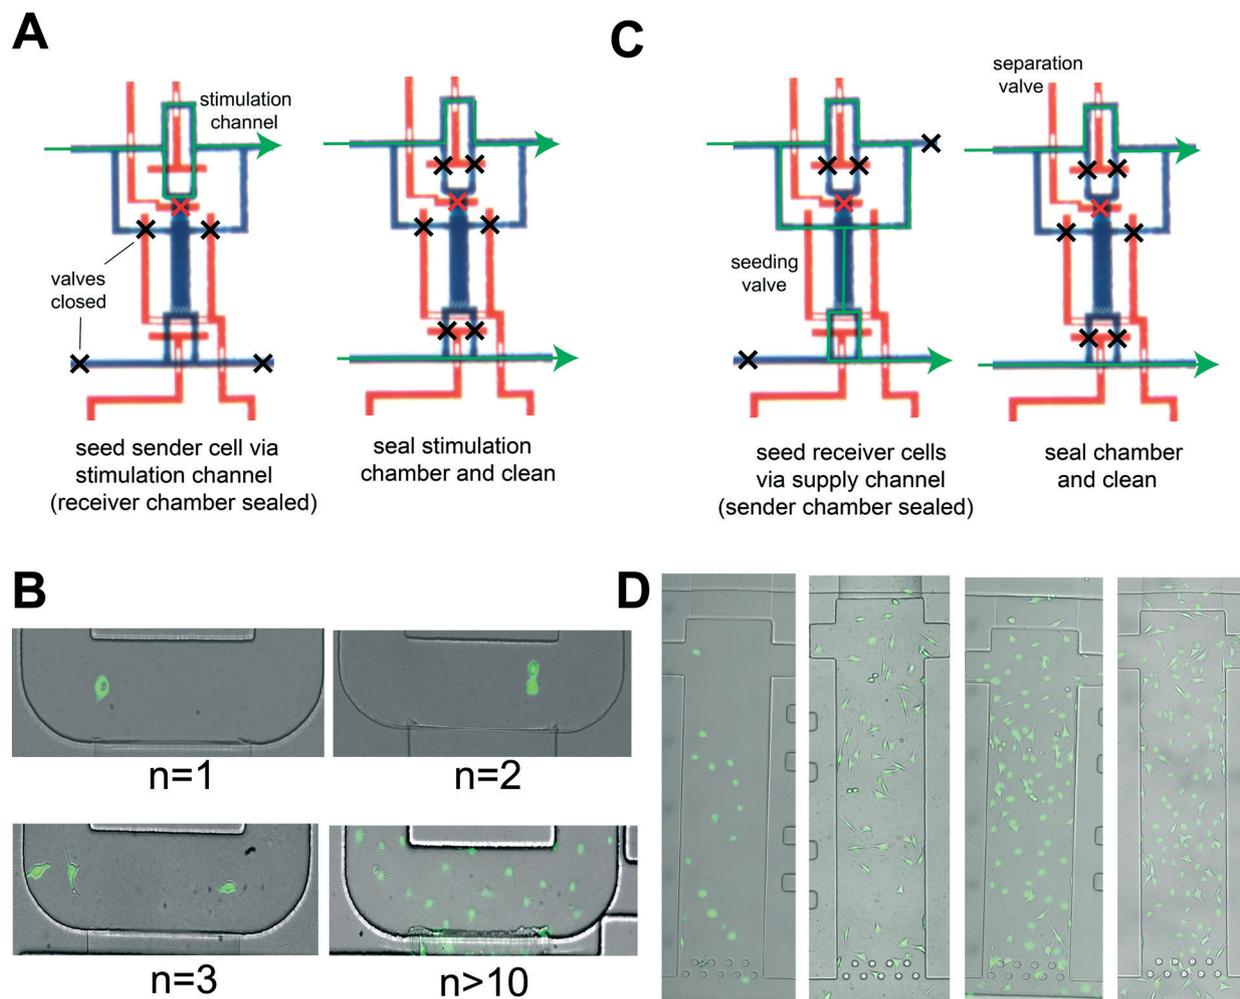


Fig. 2 (A) Sender cells (*i.e.* macrophages) are seeded *via* the upper stimulation channel (in green). After trapping cells in the sender chamber, supply channels are cleared from remaining cells by washing with fresh medium for few seconds while the seeding valve is kept closed. Crosses indicate closed valves. (B) The experimenter can control the number of sender cells. Here different numbers of macrophage cells seeded in sender chamber are shown. (C) Receiver cells (*i.e.* fibroblasts) are seeded in the receiver chamber by flowing cells from the upper supply channel through the cell culture chamber to the lower supply channel. After the desired densities of receiver cells are reached, the cell culture chamber is sealed by closing valves and the supply channels are cleared from remaining cells by flushing with fresh medium. (D) We can seed different densities of receiver cells. Density can be controlled by input suspension density. Further an iterative seeding process (seed, attach, repeat) allows fine tuning of cell density.

In vivo, the signal transmitting cells are surrounded by other tissue cells and transmit their signal radially (Fig. 1B). Spatially and temporally controlled stimulation of such a cell in the middle of other cells is a challenge. We reduced this 2-D problem to a 1-D problem by arranging the communication chain in a signalling axis that allows us to stimulate the signal-transmitting cell at will, and to send the signal in one dimension along a signalling axis by opening a separation valve (Fig. 1C). The design simplicity of the single experimental unit shown in Fig. 1D allowed us to easily up-scale our chip with six independent copies of the same unit design (Fig. 1F) in order to run different experiments in various conditions. This design is suitable for further up-scaling by using a denser arrangement of chambers to realize high-throughput devices. Our system can operate with very few numbers of

cells, which is an important advantage if rare cells from primary tissue samples are the object of investigation.

As shown in Fig. 1D the single unit consists of two culture chambers ($250\ \mu\text{m} \times 1200\ \mu\text{m} \times 25\ \mu\text{m}$, and $250\ \mu\text{m} \times 400\ \mu\text{m} \times 25\ \mu\text{m}$) that are separated by a reversible separation valve that allows quick switching from mono- to co-culture conditions (Fig. 1E). Further we can maintain the spatial position of the cultured cells in a geometrical controlled fashion, which is advantageous for computational model fitting.

Since cell-cell communication *via* paracrine signalling in tissue is a process primarily based on diffusion, we decided to culture our cells in a flow free environment, preventing any active fluid movement to influence the communication environment or wash away secreted signalling molecules. We therefore placed at the bottom as well as at the top of the

culture chamber supply channels that allow us to feed cells with fresh medium by diffusion, and remove waste products. These channels act as local source/sink for culture media. They can be seen as a microfluidic analogue of a nearby blood vessel, as suggested by Yde *et al.*²⁶

Setting up the co-culture experiment

To run a co-culture experiment, we first coat our device with fibronectin or poly-L-lysine. In order to avoid cells sticking to the supply channels, we coat them with pluronic acid (10 mg mL⁻¹). Fig. 2 shows how cells are seeded for the co-culture experiment and their final arrangement. We flow in the signal transmitting (sender) cells – cells that will see the local external input – through the top supply channel and leave the stimulation valve open. We keep the valves at the bottom supply channel closed. Sender cells only flow through the upper channel. By using low concentration of cells in the input suspension (2000 cells mL⁻¹) we can quickly trap the desired number of cells in this small chamber by opening and closing the stimulation valve (Fig. 2A). This manual seeding step enables us to seed different numbers of sender cells (Fig. 2B), from a single cell to tens of cells, without implementing different fluidic designs for each condition. Once we are satisfied with the sender cell(s) seeded, we close the stimulation valve and wash the supply channel with medium to remove all of the remaining cells.

The receivers – cells that become activated by stimulated cells – are flowed in from the top supply through the cell culture chamber to the bottom supply channel (Fig. 2C). In order to avoid receiver cells sticking in the sender cell area, we implemented a connection from the upper supply channel to the cell culture area that is controlled by the seeding valve. After cells are seeded, we close the seeding valve and flush the supply channels with medium to remove all remaining cells in the supply channel.

The density of the receiver cells in the chamber can be controlled by using different cell densities in the seeding suspension, and in the case of adherent cells repeated seeding cycles can be used as well (Fig. 2D). Once we have a certain cell number in the chambers, observed by real-time microscopy, we let the cells adhere and apply the seeding cycle a second time, until the desired density is reached. Note that every single unit of this version is independent from the others with respect to conditions. We keep the separation valve closed during the whole process, to avoid cell–cell communication.

Single-cell stimulation and co-culture

We aim to locally stimulate the sender cells without affecting the receiver cells, which is achieved by having the separation valve between the two cultures closed. As shown in Fig. 3A and Movie S1† we fill the top supply channel with the stimulus (*i.e.* bacterial LPS), then pump the fluid through the sender chamber by opening the stimulation valve and incubating the sender cell in this environment. While the input is acting on the sender cell, we can wash the supply channel or stimulate

cells in another chamber in the meantime. Once the stimulus time is over (~10 min), we wash away the stimulus with fresh medium (~1 min), and let the sender cell incubate and secrete its signalling molecules. Most cells secrete minimal amounts of signalling molecules during the stimulation time (for example, TNF secretion peaks several hours after LPS stimulation), and the removal of these molecules has a minimal impact on the total amount secreted by the sender cells.²⁷

As mentioned before, we culture our cells in a flow-free diffusion-based environment. We bring fresh medium *via* the supply channels to the chamber and fresh nutrients can diffuse from there to the cell culture area. Also waste products and signalling molecules are locally removed from the micro-environment, like in a blood vessel. Since we have six chambers in parallel and these chambers do share the same supply channel, cross-contamination has to be avoided. To fulfil this goal, we apply flow-switching mode that makes use of fast flow and slow diffusion, as previously reported.^{28,29} The flow cycles are shown in Fig. 3B. We first replace the fluid in the supply channel with fresh medium. Then we stop the flow and open the valve separating the bottom supply channel with the cell culture chamber. We use four on-chip valves (Fig. 1D) to form an on-chip peristaltic pump and pump slowly the fluid into the chamber. Typically, we replace the medium for 5 seconds and pump for 25 seconds at a frequency of 10 s⁻¹. This switch between fast replacement of the medium in the channel and bringing fresh medium slowly to cells helps us to avoid flow over the cells. We simulated the influence of slow flow in the chamber (Fig. 3C). These simulations reveal that the flow remains mainly in the supply channels and does not reach the cell culture area at small flow rates used in this study.

An LPS stimulated macrophage spatiotemporally controls NF-κB activation in fibroblasts

The NF-κB pathway is a major innate immune signalling network that recognizes pathogenic or self-secreted signalling molecules. Upon pathway activation, the inhibitors of NF-κB are degraded, allowing NF-κB transcription factors (like p65) to translocate to the nucleus and activate response genes. These response genes regulate cell physiology, and lead to further secretion of signalling molecules to establish cell–cell communication and ultimate removal of pathogenic cells. Previously, time-dependent analysis of NF-κB activity in single cells enabled quantitative and accurate understanding of immune signalling and allowed its comprehensive modelling.^{8,9,30,31} Prior to this work, however, the spatial aspects of NF-κB signalling have been addressed in very few studies,^{13,26,32} and one-way communication between signal sending and receiving cells has not been studied in a controlled way due to technical limitations in generating localized signals within co-culture conditions.

Here, we used our device to implement a co-culture scenario that mimics the initiation of an inflammatory process induced by bacterial infection. As a local environmental input we used LPS, a product emitted from the cell wall of Gram-

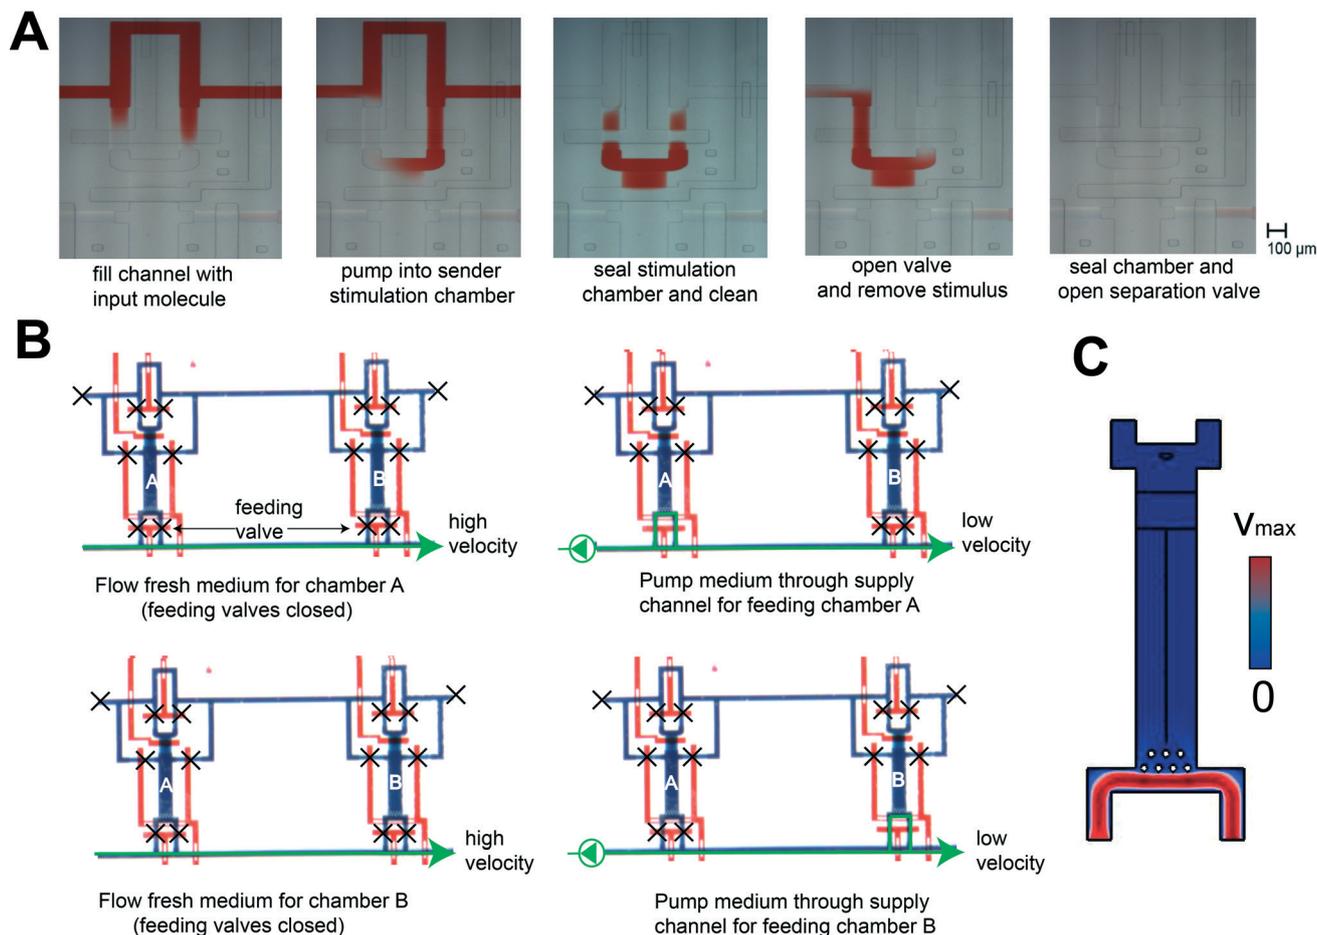


Fig. 3 (A) Stimulation starts by filling the upper flow supply channel with the stimulus. Next we gently pump the stimulus into the sender chamber. We then close the stimulation valve and wash away the stimulus in the supply channel. After the stimulation time is over the sender cell chamber is washed until the chamber is cleared from the stimulus. (B) Cells are fed *via* diffusion from the lower supply channel. First, we flush the supply channel with fresh medium for 5 seconds while the valves separating cell culture chambers from supply channels are kept closed. We then open a cell culture chamber while the neighbouring chambers are still closed to avoid cross-contamination. We then pump slowly fresh medium to the edge cell culture chamber for 25 seconds at a frequency of 10 Hz. The chamber is then disconnected from the supply channel by closing the valve and waste products are removed by flushing fresh medium for 5 seconds. The next chamber is then fed as before. Once all chambers were addressed, the procedure repeats. (C) We simulated the influence of the feeding flow to the cell chamber in COMSOL. We used the same chamber geometry and $100 \mu\text{m s}^{-1}$ as input flow velocity. The heat plot indicates that flow does not reach inside the chamber and cells will not be affected by flow.

negative bacteria like *E. coli*.³³ This LPS input acts on the macrophage, a specialized first responder cell, that in turn activates NF- κ B signalling through binding of LPS to the TLR4 receptor.³⁴ As a response, the macrophage produces and secretes the inflammatory cytokine TNF, which is sensed by nearby tissue cells, in this case 3T3 fibroblasts. These fibroblasts will then activate NF- κ B signalling *via* TNF/TNFR binding (Fig. 4A). Through ELISA measurements we have ensured that our macrophage cells do not respond to self secreted TNF, and that our fibroblast cells do not produce TNF upon NF- κ B stimulation (data not shown), which allowed us to create a one-way (macrophage to fibroblast) communication scenario.

In these experiments, we seeded a single macrophage in the sender chamber and placed a dense colony of fibroblasts in the receiver chamber below, each expressing a fluorescent

protein (GFP or DsRed) fused to p65, the main subunit of NF- κ B in mouse cells. The macrophage was then stimulated with two 10 minute pulses of LPS ($c = 50 \text{ ng mL}^{-1}$) with a 10 minute break in between (Fig. 4B), simulating repeated exposure to bacteria. The LPS was then washed away for 1 minute and the separation valve was opened, allowing secreted TNF to diffuse over the fibroblast colony and activate NF- κ B. The fluorescent fusion proteins in our cells allowed us to measure NF- κ B activity (cytoplasm-nuclear translocation) in real-time using automated live-cell microscopy (Fig. 4C). To ensure that the observed signal is not due to left-over LPS in the top chamber, we filled the top chamber with LPS and washed it away for 1 minute as in signalling experiments. When this chamber was exposed to the fibroblasts no activation was seen, showing that LPS is efficiently washed away from the macrophage chamber (Fig. S1†). To test if TNF is the main

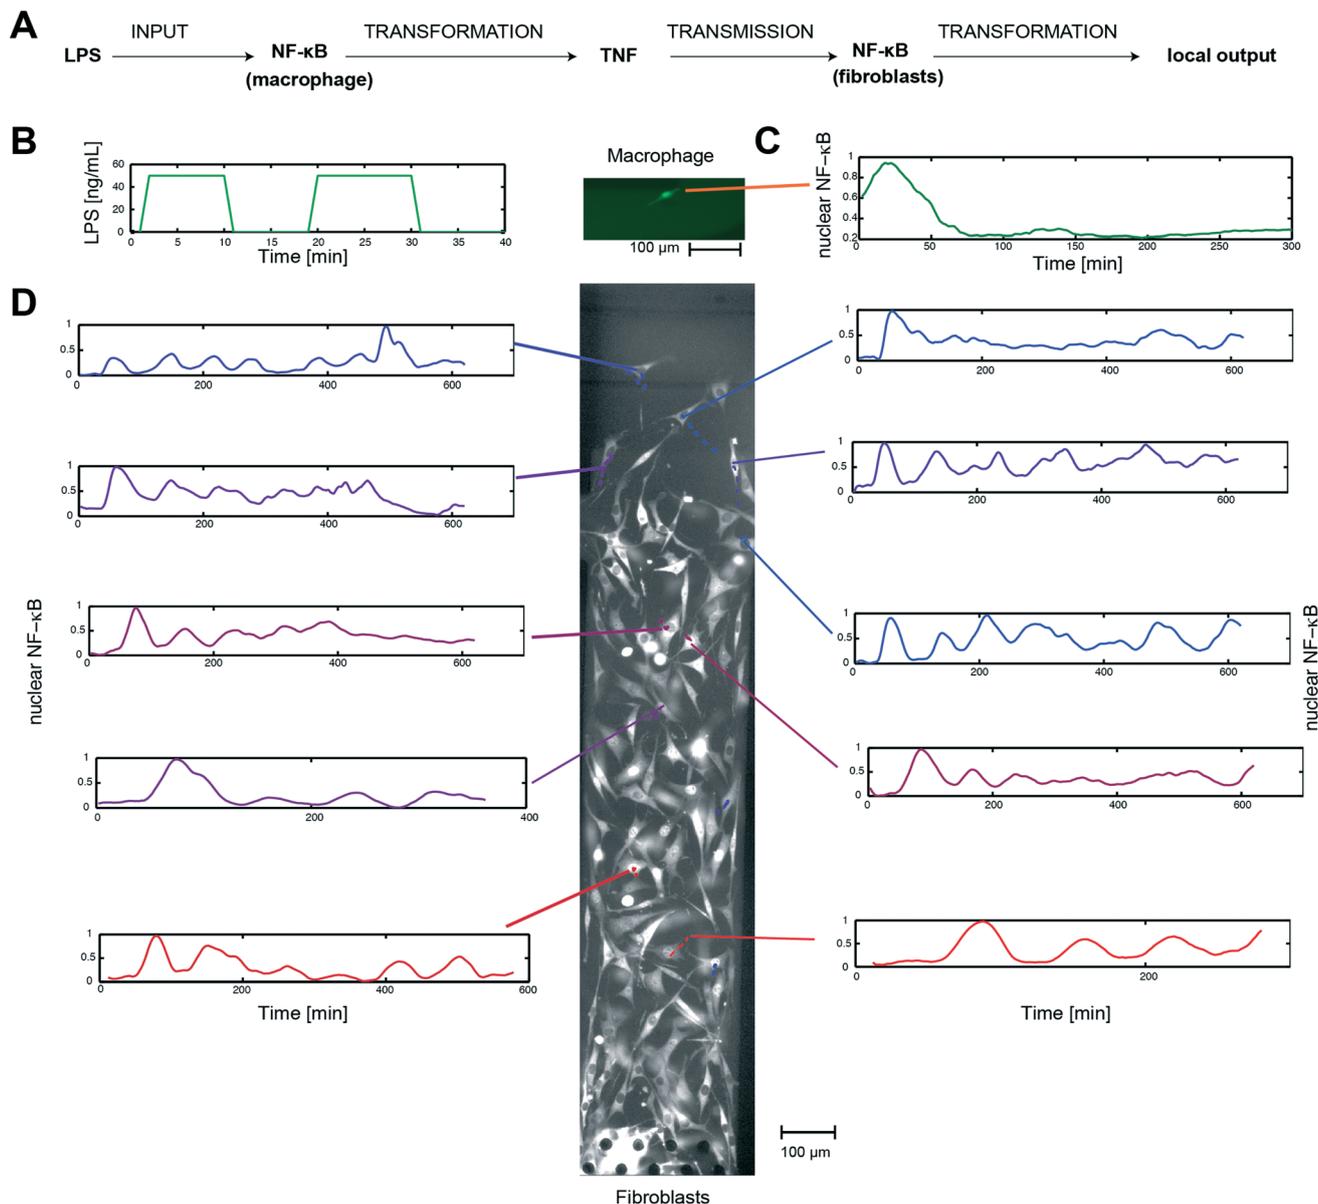


Fig. 4 (A) One-way communication chain mimicking an inflammatory process. LPS acts as initiator on macrophages that in turn activate NF- κ B signalling. This input is then transformed to a TNF secretion response and transmitted to fibroblasts. These fibroblasts transform TNF information via a NF- κ B signal to a local output. (B) We locally stimulated a macrophage with two 10 minute pulses of 50 ng mL^{-1} LPS, with a 10 minute break in between, before exposing the macrophage to the fibroblasts. (C) Macrophage NF- κ B time course upon LPS stimulation. The picture shows the LPS activated macrophage, since the GFP labelled p65 marker is accumulated in the nucleus. (D) Single-cell map of fibroblast NF- κ B responses with respect to time and space. The secretion product of the macrophage (mainly TNF) initiates sustained and spatially patterned signalling in these cells. The dashed lines represent the nuclear locations of the cells during the experiment. The picture shows the DsRed labelled NF- κ B (p65) of fibroblasts. Cells are activated if the p65 accumulated in the nucleus. Otherwise it remains in the cytosol. Mean nuclear p65 intensities are normalized to the maximum of the highest peak.

secretion product that activates NF- κ B in our fibroblasts, we stimulated a macrophage with LPS and co-cultured it with fibroblasts with TNF-antibody added to the culture medium. Compared to the experiment without TNF-antibody, we observed no NF- κ B activation in fibroblasts, since the antibody captured all the TNF molecules in the medium (Fig. S2[†]). This shows that TNF is the main NF- κ B signal mediator secreted by the LPS activated RAW macrophage. Further, we have not observed cell cycle dependent oscillations in the

fibroblast cells. We also co-cultured one macrophage with a population of fibroblast without LPS stimulation, but did not observe spatially organized signal activation. Nevertheless, one or two cells showed weak NF- κ B activation (Fig. S3[†]), which can arise spontaneously among dense cultures.³⁵

Our fibroblasts have a nuclear marker (H2B-GFP) that allows us to automatically track them using live-cell-microscopy. Using our chip, we were able to establish the one-way communication scenario described above and measure NF-

κ B dynamics in both signal sending and receiving cells, and mapped the spatiotemporal distribution of single cell immune response to bacterial infection for the first time. We observed an NF- κ B activation pattern propagating from the signal sending macrophage into the fibroblast population (Fig. 4D, Movie S2†). The macrophage emitted immune signal reached most of the fibroblast cells, with farther away cells showing a time-delayed activation profile and fewer NF- κ B oscillations. Since NF- κ B dynamics controls gene expression in fibroblasts, one can expect to see differential target gene expression in the responding fibroblast population depending on their distance from the macrophage.⁸ This observed spatiotemporal signalling pattern demonstrates that the cytokine secretion time-course of one single macrophage cell can activate and control over 100 single fibroblast cells that are up to 1 mm away from the secreting cell. The NF- κ B oscillations lasted up to 10 hours in some fibroblasts, showing that a brief (20 minute) exposure to a pathogenic signal like LPS can induce a long-term inflammatory response in the nearby tissue cells.

Conclusions

We developed a novel automated microfluidic co-culture device and live-cell imaging system that allows us to address questions in signal transduction with respect to space and time. We can locally induce a chemical signal in single immune cells and measure how secondary signals emitted by activated immune cells propagate in space through a population of signal receiving tissue cells. Traditionally, co-culture experiments are conducted as population–population^{36–38} or pairwise single-cell interaction,^{39,40} but we establish a signalling scenario between a single cell and a dense population. Our microfluidic device does not require the integration of complicated systems like optical or magnetic tweezers for signal delivery^{18,19} and can overcome introducing several genetic constructs to conduct spatiotemporal signalling.¹³

We established macrophage/fibroblast co-culture experiments on our system and measured spatiotemporal signalling of NF- κ B in single cells. We simulated an inflammatory scenario on chip and found that a local LPS input is converted into a spatiotemporal NF- κ B activation profile. This device will allow detailed, precise and quantitative investigation of how inflammation is controlled by gene network dynamics, and how gene expression patterns are established in inflamed tissue. Together with mathematical modelling, we will be able to model spatiotemporal aspects of immune signalling and understand innate immunity better, particularly with respect to chronic diseases, and confirm model predictions experimentally using this simple yet effective platform.

Acknowledgements

We would like to thank Erica Montani and Thomas Horn from the BSSE Single Cell Facility for technical support. This work

was funded by an ERC Starting Grant (SingleCellDynamics) to ST, Swiss National Science Foundation (SNF), SNF Systems X (NeuroStemX), and NCCR Molecular Systems Engineering.

Notes and references

- 1 A. C. Chiang and J. Massagué, *N. Engl. J. Med.*, 2008, **359**, 2814.
- 2 S. Shimozono, T. Iimura, T. Kitaguchi, S. Higashijima and A. Miyawaki, *Nature*, 2013, **496**, 363.
- 3 Y. F. Hu, J. F. Dawkins, H. C. Cho, E. Marbán and E. Cingolani, *Sci. Transl. Med.*, 2014, **6**, 245ra94.
- 4 B. M. Ahmer, *Mol. Microbiol.*, 2004, **52**, 933.
- 5 E. L. Stern, N. Quan, M. G. Proescholdt and M. Herkenham, *J. Neuroimmunol.*, 2000, **109**, 245–260.
- 6 A. Hoffmann and D. Baltimore, *Immunol. Rev.*, 2006, **210**, 171.
- 7 S. Nahavandi, S.-Y. Tang, S. Baratchi, R. Soffe, S. Nahavandi, K. Kalantar-Zadeh, A. Mitchell and K. Koshmanesh, *Small*, 2014, **10**, 4810.
- 8 S. Tay, J. J. Hughey, T. K. Lee, T. Lipniacki, S. R. Quake and M. W. Cover, *Nature*, 2010, **466**, 267.
- 9 R. Kellog and S. Tay, *Cell*, 2015, **160**, 381.
- 10 F. Guo, J. B. French, P. Li, H. Zhao, C. Y. Chan, J. R. Fick, S. J. Benkovic and T. J. Huang, *Lab Chip*, 2013, **13**, 3152.
- 11 B. Sun, J. Lemborg, V. Normand, M. Rogers and H. A. Stone, *Proc. Natl. Acad. Sci. U. S. A.*, 2012, **109**, 7753.
- 12 H. Youk and W. A. Lim, *Science*, 2014, **343**, 1242782.
- 13 T. K. Lee, E. M. Denny, J. C. Sanghvi, J. E. Gaston, N. D. Maynard, J. J. Hughey and M. W. Covert, *Sci. Signaling*, 2009, **2**, ra65.
- 14 O. Wartlick, P. Mumcu, A. Kicheva, T. Bittig, C. Serum, F. Jülicher and M. González-Gaitán, *Science*, 2011, **331**, 1154.
- 15 T. Lämmermann, P. V. Alfonso, B. R. Angermann, J. M. Wang, W. Kastenmüller, C. A. Parent and R. N. Germain, *Nature*, 2013, **498**, 371.
- 16 A. J. Müller, O. Filipe-Santos, G. Eberl, T. Aebischer, G. F. Späth and P. Buosso, *Immunity*, 2012, **37**, 147.
- 17 S. Vedel, S. Tay, D. Johnston, H. Bruus and S. R. Quake, *Proc. Natl. Acad. Sci. U. S. A.*, 2013, **110**, 129.
- 18 E. D'Este, G. Baj, P. Beuzer, E. Ferrari, G. Pianto, E. Tongiorgi and D. Cojoc, *Integr. Biol.*, 2011, **3**, 568.
- 19 D. Fan, Z. Yin, R. Cheong, F. Q. Zhu, R. C. Cammarata, C. L. Chien and A. Levchenko, *Nat. Nanotechnol.*, 2010, **5**, 545.
- 20 C. Beta, D. Wyatt, W.-J. Rappel and E. Bodenschatz, *Anal. Chem.*, 2007, **79**, 3940.
- 21 G. Gerisch and H. U. Keller, *J. Cell Sci.*, 1981, **52**, 1.
- 22 V. V. Abhyankar and D. J. Beebe, *Anal. Chem.*, 2007, **79**, 4066.
- 23 G. A. Cooksey, C. G. Sip and A. Folch, *Lab Chip*, 2009, **9**, 417.
- 24 P. Chang, P. Cheng, X. Feng, W. Dei and B.-F. Lin, *Anal. Bioanal. Chem.*, 2013, **405**, 307.
- 25 R. Kellogg, R. Gómez-Sjöberg, A. A. Leyart and S. Tay, *Nat. Protoc.*, 2014, **9**, 1713.
- 26 P. Yde, B. Mengel, M. H. Jensen, S. Krishn and A. Trusina, *BMC Syst. Biol.*, 2011, **5**, 115.

- 27 A. J. Torres, R. L. Contento, S. Gordo, K. W. Wucherpfennig and J. C. Love, *Lab Chip*, 2013, 13, 90.
- 28 T. Frank and S. Tay, *Lab Chip*, 2013, 13, 1273.
- 29 M. Mehling, T. Frank, C. Albayrak and S. Tay, *Lab Chip*, 2015, 15(5), 1276–1283.
- 30 A. Hofmann, A. Levchenko, M. L. Scott and D. Baltimore, *Science*, 2002, 298, 1241.
- 31 J. J. Hughey, M. V. Gutschow, B. T. Bajar and M. W. Covert, *Mol. Biol. Cell*, 2015, 26(3), 583–590.
- 32 C. A. Kaspar, I. Sorg, C. Schmutz, T. Tschon, H. Wischnewski, M. L. Kim and C. Arriermerlou, *Immunity*, 2010, 33, 804.
- 33 C. R. H. Raetz and C. Whitfield, *Annu. Rev. Biochem.*, 2002, 71, 635.
- 34 M. Baer, A. Dillner, R. C. Schwartz, C. Sedon, S. Nedospasov and P. F. Johnson, *Mol. Cell. Biol.*, 1998, 18, 5678.
- 35 J. Pekalski, P. J. Zuk, M. Kochanczyk, M. Junkin, R. Kellog, S. Tay and T. Lipniacki, *PLoS One*, 2013, 8, e78887.
- 36 D. J. Holt, L. M. Chamberlain and D. W. Grainger, *Biomaterials*, 2010, 31, 9382.
- 37 L. Goers, P. Freemont and K. M. Polizzi, *J. R. Soc., Interface*, 2014, 11, 20140065.
- 38 M. B. Byrne, L. Trump, A. V. Desai, L. B. Schook, H. R. Gaskin and P. J. A. Kenis, *Biomicrofluidics*, 2014, 8, 044104.
- 39 Z. Yin, D. Noren, C. J. Wang, R. Hang and A. Levchenko, *Mol. Syst. Biol.*, 2008, 4, 232.
- 40 S. Hong, Q. Piong and L. P. Lee, *Integr. Biol.*, 2012, 4, 374.